

For Use Under an Emergency Use Authorization (EUA) Only
For *in vitro* diagnostic use



cue

User Manual

Cue™ Health Monitoring System

User Manual

Basic Information

Please read this User Manual carefully. Contact Cue Health Customer Support at support@cuehealth.com or call toll-free at (833) CUE-TEST · (833) 283-8378 if you have any questions or comments.

Cue Health Inc.

San Diego, CA 92121

www.cuehealth.com

Cue™ is a trademark of Cue Health Inc.

Table of Contents

Chapter 1 - Introduction and User Safety	7
Welcome to Cue	7
Intended Use	7
Before Testing with the Cue Health Monitoring System.....	8
Safety Definitions	9
Practices Used in This User Manual	11
Symbols and Descriptions.....	12
General Precautions.....	14
Chapter 2 - Cue Health Monitoring System	
Overview and Features.....	16
Cue Health Monitoring System Components.....	17
Cue Health Monitoring System Package Contents	19
Cue Test Cartridge Pack	20
Compatible Mobile Smart Devices	22
Cue Health App	22
Accessories Available Separately	23

Table of Contents

Chapter 3 - Setting Up Your Cue Health

Monitoring System.....	24
Identifying Parts of Your Cue Cartridge Reader.....	24
Your Cue Health App Dashboard	27
Cue Cartridge Reader Indicator Lights	28
Downloading and Installing the Cue Health App	30
Creating Your Cue Account and User Profile	32
Setting Up the Cue Cartridge Reader	35
Account Login	40

Chapter 4 - Running a Test on the Cue Cartridge

Reader	41
Reasons for Incorrect or Invalid Results.....	43
Initiate Test.....	44

Table of Contents

Chapter 5 - Cue Health Monitoring System

Management	46
Charging the Cue Cartridge Reader	46
Account Settings	48
Pairing Additional Cue Cartridge Readers to Your Mobile Smart Device	49
Connecting the Cue Cartridge Reader to the Cue Health Mobile App.....	50
Checking the MAC Address of a Connected Cue Cartridge Reader.....	51
Disconnecting the Cue Cartridge Reader from the Cue Health App.....	52
Unpairing the Cue Cartridge Reader from Your Mobile Smart Device	54
Managing User Account and Profiles.....	55
Forgot Your Password?.....	57
Printing Your Test Results.....	58
Accessing Product Documentation	60

Table of Contents

Chapter 6 - Cleaning and Disinfecting	61
Cleaning and Disinfecting.....	61
Chapter 7 - Troubleshooting	63
Error Messages and Recommended Actions	64
When to Use the Manual Reset Button	66
Chapter 8 - Technical Information and Specifications	67
How the Cue Health Monitoring System Works.....	67
Technical Specifications	68
Compliance with International Standards	69
Disposing of Your Cue Health Monitoring System and Components	70
Chapter 9 - Warranty and Supplies	71
Manufacturer's One Year Warranty	71
Supplies and Accessories	71

Chapter 1

Introduction and User Safety

Welcome to Cue

The Cue Health Monitoring System is a fast and easy to use system for performing medical tests. Your results are delivered and saved to a mobile smart device in minutes. This User Manual will guide you through the proper setup and use of the Cue Health Monitoring System. Read this manual thoroughly to help you understand the system and its many features.


Intended Use

The Cue Health Monitoring System is an in vitro diagnostic medical device for use with test-specific Cue Cartridge(s) and the Cue Health Mobile Application (Cue Health App) installed on a mobile smart device such as the Apple® iPhone® 8+ or later with iOS 13 or later.

Before Testing with the Cue Health Monitoring System

Review the Quick Start Guide and this User Manual before you run a test using the Cue Health Monitoring System.

The Quick Start Guide will help you quickly set up your system and get ready to run a test. This User Manual gives you all the information you need to use your system correctly and safely.

 ***It is important that you follow the instructions in this User Manual. If you do not use the system correctly, you may get an incorrect or invalid result, the system may cancel your test, or you may damage the system. Do not use the system if you cannot follow the instructions.***

If you have any questions, please contact Cue Health Customer Support at support@cuehealth.com or call toll-free at (833) CUE-TEST · (833) 283-8378.

Safety Definitions

This User Manual includes three types of important messages. They are Warnings, Cautions, and Notes. It is important that you pay close attention to these messages to make sure you use the Cue Health Monitoring System correctly and safely.



Warning

A Warning message tells you what you need to do to prevent possible risk of injury or damage to your health.

Follow the instructions given when you see a Warning message. Do not proceed if you do not fully understand the actions to take after seeing a Warning message.



Caution


A Caution message tells you what you need to do to prevent damage to your Cue Health Monitoring System. Do not proceed if you do not fully understand the actions to take after seeing a Caution message.



Note

A Note is used to give you more information to make the instructions clearer.

Practices Used in This User Manual

Procedure steps in this User Manual are easy to find. They begin with a  symbol, followed by a short description of the action to be performed.







Procedure steps are numbered and should be performed in that order.





When there is a system response to the procedure step performed, it appears in italics below the procedure step.

Words in:	Description
Bold	Names of menus and buttons
<i>Italics</i>	System response that occurs as a result of pressing an icon or an action command in the Cue Health App
<i>Bold Italics</i>	Used to emphasize important information

Symbols and Descriptions

The table below describes the symbols used on the Cue Health Monitoring System packaging and on the system parts.

Symbol	Description
	Consult User Manual
	Serial Number
	Do not use if seal or packaging is broken or damaged
	Storage temperature range
	Humidity Storage range
	Catalog number

Symbol	Description
	Manufacturer
	Keep dry
	Electrical and Electronic Equipment Waste: Discard product at separate collection facility for recovery and recycling.
	Caution: Indicates the need for the user to consult the instructions for use for important cautionary information such as warnings and precautions that cannot, for a variety of reasons, be presented on the medical device itself.

General Precautions

The Cue Health Monitoring System may not work correctly if there is damage to the package or the system parts.

- Do not use the Cue Health Monitoring System if the package seals are broken.
- Do not use Cue Health Monitoring System if any part is damaged.
- Do not run a test if the room temperature is outside of the testing conditions stated in the test-specific Cue Cartridge Instructions for Use. Testing in room temperatures that are too high or too low may cause an incorrect or invalid result.
- Do not use the Cue Health Monitoring System in altitudes higher than 8530 feet (2600 meters). Testing at altitudes that are too high may cause an incorrect or invalid result.
- Do not leave the Cue Health Monitoring System in temperatures below 39°F (4°C) or above 100°F (38°C).
- If you make changes to any of the parts of your Cue Health Monitoring system or use any parts that did not come with the system, you may harm yourself and the system. You will also void your warranty.

- The Cartridge Reader should be placed on a stable, flat, and level surface while running a test. Do not move or tilt the Reader while a test is in progress.
- This product has not been FDA cleared or approved.
- This product has been authorized by FDA under an EUA for use by laboratories certified under the Clinical Laboratory Improvement Amendments of 1988 (CLIA), 42 U.S.C §263a, to perform moderate complexity/high complexity tests and at the Point of Care (POC), i.e., in patient care settings operating under a CLIA Certificate of Waiver, Certificate of Compliance, or Certificate of Accreditation.
- This product has been authorized only for the detection of nucleic acid from SARS CoV-2, not for any other viruses or pathogens.
- This product is only authorized for the duration of the declaration that circumstances exist justifying the authorization of emergency use of in vitro diagnostic tests for detection and/or diagnosis of COVID-19 under Section 564(b)(1) of the Act, 21 U.S.C §360bbb-3(b)(1), unless the authorization is terminated or revoked sooner.




Chapter 2

Cue Health Monitoring System Overview and Features

The Cue Health Monitoring System include three parts. These parts include the Cue Cartridge Reader, the Cue Power Adapter, and the Cue Charging Cable. The Cue Wireless Charging Base is available as an optional part (accessory). The Cue Health Monitoring System is used with test-specific Cue Cartridges and sample collection devices (Cue Sample Wand). The Cue Cartridge Reader connects to the Cue Health App installed on your Apple iPhone 8+ or later device. The iPhone mobile smart device is the primary display for the test system.

Cue Health Monitoring System Components

Each Cue Health Monitoring System part (component) is described in the table on the next page.

Component	Description	Image
Cue Cartridge Reader	The Cue Cartridge Reader communicates with the Cue Health App and the test-specific Cue Cartridges to run a test on a sample.	
Cue Power Adapter	The Cue Power Adapter plugs into standard wall power. The Cue Charging Cable plugs into the Cue Power Adapter.	
Cue Charging Cable	The Cue Charging Cable connects the Power Adapter to the Cartridge Reader.	

Cue Health Monitoring System Package Contents



Make sure that your system contains the following parts (components):

- One (1) Cue Cartridge Reader
- One (1) Cue Power Adapter
- One (1) Cue Charging Cable
- User Manual
- Quick Start Guide

Contact Cue Health Customer Support at support@cuehealth.com or call toll-free at (833) CUE-TEST · (833) 283-8378 if you do not have all of these parts. Also contact Cue Health Customer Support if a part is damaged.

Cue Test Cartridge Pack

The table on the next page describes Cue Test Cartridge Packs. Cue Test Cartridge Packs are available for different tests including a test for SARS-CoV-2 virus (COVID-19). Cue Test Cartridge Packs are sold separately and must be used before the Use By date printed on the cartridge pack label.

Component	Description	Image
<p>Cue Test Cartridge Pack</p>	<p>A Cue Test Cartridge Pack comes with a Cue test cartridge, a Cue Sample Wand for collecting a sample, and Instructions for Use. The Instructions for Use tell you how to use the Cue Cartridge Reader, the Cue Health App, and the Cue cartridge to run a test on the sample.</p>	 <p>Cue COVID-19 Test Cartridge</p>  <p>Cue Sample Wand</p>

Compatible Mobile Smart Devices

The Cue Health Monitoring System may be used with iPhone 8+ or later models. The operating system on the iPhone 8+ or above must be iOS 13 or later.

Cue Health App


The Cue Health App is required to run the Cue Health Monitoring System. Download the Cue Health App from the Apple App Store®.

The Cue Health App displays test results from the Cue Health Monitoring System. The Cue Health App must be open to see test results.

If the mobile smart device loses power, the test on the Cue Health Monitoring System will still run to completion. The result will not be displayed until the mobile smart device is charged. Bring the charged mobile smart device close to the Cue Cartridge Reader and open the Cue Health App to see the test result.

The Cue Health App also stores test results and communicates with the internet and the secured cloud storage.

Accessories Available Separately


Component	Description	Image
Cue Wireless Charging Base	The Cue Cartridge Reader may be charged wirelessly using the Cue Wireless Charging Base. The Cue Cartridge Reader is secured by magnets when charging on top of the Cue Wireless Charging Base.	 A white, rectangular wireless charging base with a square charging pad on top and a small port on the side.

Chapter 3

Setting Up Your Cue Health Monitoring System


Identifying Parts of Your Cue Cartridge Reader

The Top and Front of Your Cue Cartridge Reader

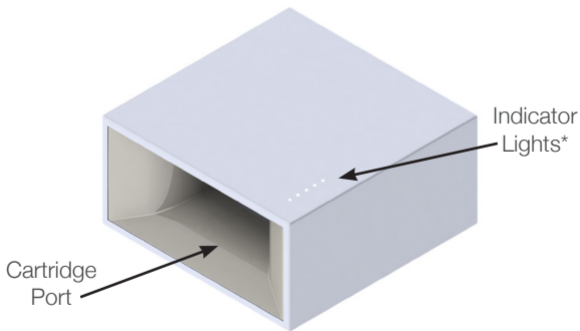

*See "Cue Cartridge Reader Indicator Lights" in Chapter 3 for information on the meaning of the indicator light patterns.

The Back of Your Cue Cartridge Reader

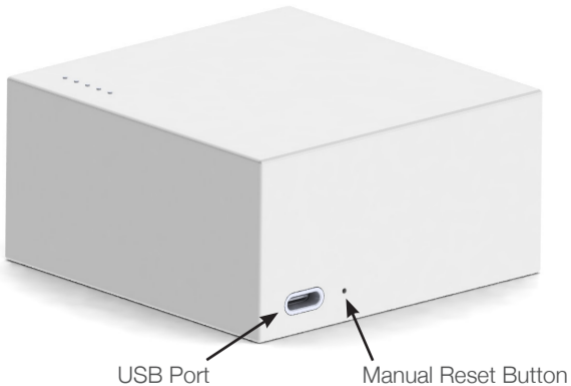

The Bottom of Your Cue Cartridge Reader



Cartridge Reader


REF: C0201

S/N: 21802010000481

L9000207-2 Rev 1.0



Your Cue Health App Dashboard

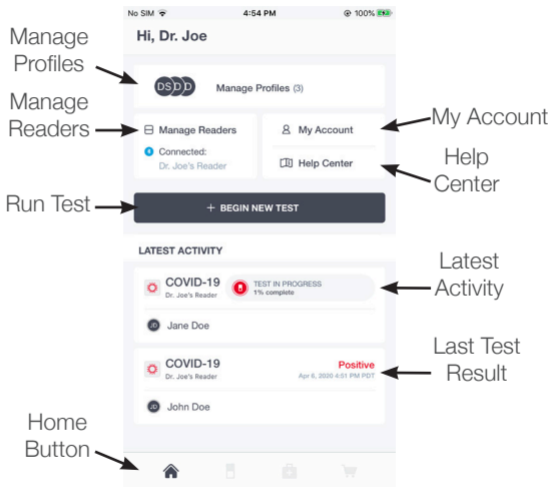

Press the Home Button  on the Cue Health App screen to see the Cue Dashboard.

Cue Cartridge Reader Indicator Lights Status Indicators

You will see different light patterns on top of the Reader. The light patterns will tell you when the Reader is connected to the Cue Health App. The light patterns will also tell you when a cartridge is inserted, and when there is an error.



Lights Flash when connected



Lights Flash when the Cue Cartridge or the Cue Sample Wand is inserted



Error, see Cue Health App for details

Prompts for an Action

You will see these light patterns on top of the Reader after you insert a Cue Cartridge into the Cartridge Port.



Insert Sample Wand with collected specimen into the Cue Cartridge



Remove Cue Cartridge (with Sample Wand inside) from the Cue Cartridge Reader

Downloading and Installing the Cue Health App

You can download and install the Cue Health App to your iPhone mobile smart device from the Apple App Store. The Cue Health App is downloaded and installed the same way as other apps on your mobile smart device. The Cue Health App is free of charge.



Cue Health


 Downloading the Cue Health App from the App Store requires internet connectivity.


 Download the Cue Health App:

1. Turn on your mobile smart device.
2. Confirm your mobile smart device has internet connectivity.


3. Launch the Apple App Store app.
4. Search for the “Cue Health App” by Cue Health Inc. and tap on the Cue Health App icon.
5. Tap Install.
6. Enter your App Store password information as required.

The application downloads. Once installed, the Cue Health App icon appears on your mobile smart device home screen.

 The Cue Health App needs to be installed on each mobile smart device.

 Cue Health App updates must be downloaded from the Cue Health App Store when a new version is available.

Creating Your Cue Account and User Profile

 *Your test results will be saved to your Cue Account and in a secured cloud storage.*

 To Create your Cue Account and User Profile:

1. Launch the “**Cue Health App**” on your mobile smart device.

The “Login” screen will be displayed by the Cue Health App.

2. Tap on “**Create Account**”.
3. Input your email and create a password on the “Create Account” screen. Continue following the on-screen instructions. You must accept the End User License Agreement and Privacy Policy.


At the completion of account creation, the “Profile Information” screen will be displayed by the Cue Health App.

4. At “Profile Information” screen, input the requested information in each field.
5. Tap on “**SUBMIT**” and follow the on-screen instructions.

At the completion of profile creation, the “Permissions” screen will be displayed by the Cue Health App.

6. Follow the Cue Health App on-screen instructions to progress through the “Permissions” screens.

After progressing through the “Permissions” screens, the “Set Up the Cue Cartridge Reader” screen will be displayed by the Cue Health App.


 *Multiple User Profiles can be created under one Cue Account. The primary Cue Account holder will have access to all User Profiles and test results under the same Cue Account.*

Setting Up the Cue Cartridge Reader

 To Set Up your Cue Cartridge Reader:

After creating a Cue Account, the “Set Up the Cartridge Reader” screen will be displayed by the Cue Health App.

1. Place the Cue Cartridge Reader on top of a stable, flat, and level surface.
2. Connect the Cue Charging Cable to the Cue Power Adapter and plug the Power Adapter into wall power.
3. Follow the Cue Health App Instructions.

 ***Only use Cue-supplied Charging Cable and Power Adapter.***

4. Wake the Cue Cartridge Reader by connecting it to the Cue Charging Cable.

When the Cue Cartridge Reader is connected to power, the lights on top of the Reader will illuminate one-by-one. The lights will then flash to show charge level. The Reader is now ready for pairing with a mobile smart device.



Another way to wake the Cue Cartridge Reader is by disconnecting and reconnecting the Cue Charging Cable. You can also wake the Reader by placing it on top of the Cue Wireless Charging Base. Make sure the Cue Wireless Charging Base is connected to wall power.


5. In the “Set Up the Cartridge Reader” screen in the Cue Health App, tap on “**SCAN NOW**” to begin pairing the Cartridge Reader to the mobile smart device.
6. Turn your Cue Cartridge Reader upside-down so the bottom of the Cue Cartridge Reader is facing up. You will see the serial number and QR code.


7. Move the mobile smart device until you can see the QR code inside of the focus square on the camera screen.



If the QR code does not scan quickly, make sure the Cartridge Reader is connected to power.


When the QR code is recognized, the Cue Health App will display a message that says, “Reader Authorized Successfully”. This means that the Cue Cartridge Reader is paired securely to the mobile smart device. The Cue Dashboard will then be displayed on the screen. Make sure to turn the Cartridge Reader over to top-side up after reading the QR code. The side with the lights on top of the Reader is top-side up.

 “Pairing” a Cartridge Reader is scanning the QR Code found on the bottom of the Reader. When a “Paired” Cartridge Reader is within Bluetooth® range of the smart mobile device, the Reader is “Connected” to the Cue Health App on the smart mobile device.

 If the camera scan of the Reader QR code does not work, the Cue Health App will let you to manually enter the Cartridge Reader MAC address and Pin Number. The MAC address and Pin are on the bottom of the Reader. See “Identifying Parts of Your Cue Cartridge Reader” in Chapter 3 for how to find the MAC address and Pin Number.

 One Cue Cartridge Reader can pair with multiple mobile smart devices.

 One mobile smart device can pair with multiple Cue Cartridge Readers.

 When you choose a paired Cue Cartridge Reader to run a test, that Reader is connected to the Cue Health App. One Cue Cartridge Reader can only connect with the Cue Health App on one mobile smart device at one time.

 Multiple Cue Cartridge Readers can be connected to the Cue Health App on one mobile smart device at one time.

Account Login

If you already have a Cue Account, you can log in directly. If you do not have a Cue Account, see “Creating Your Cue Account and User Profile” in Chapter 3 for instructions on how to set up a Cue Account.

 To Log In:

1. Launch the “**Cue Health App**” on your mobile smart device.

The “Login” screen will be displayed by the Cue Health App.


2. Input your Email and Cue Account Password.
3. Tap on “**LOGIN**”.


The “Dashboard” screen will be displayed by the Cue Health App after login.


Chapter 4

Running a Test on the Cue Cartridge Reader

Carefully read this chapter. It is important that you read and follow the test-specific instructions for Use found inside the Test Cartridge Pack box, electronically in the Help Center of the Cue Health App, or at www.cuehealth.com

 ***If you do not follow all of the instructions you may get an incorrect or invalid result.***

 ***The Cartridge Reader should be placed on a stable, flat, and level surface while running a test. Do not move or tilt the Reader while a test is in progress.***

 The Cue Health App will tell you if the Cartridge Reader battery is too low to complete a test. Connect the Reader to power when needed.



If your mobile smart device loses battery charge, the test on the Cartridge Reader will still run to completion. The test result will be saved. The mobile smart device must be charged to see the test result. Make sure your mobile smart device is close to the Cartridge Reader after a test completes so you can view your result on the screen in the Cue Health App.

Reasons for Incorrect or Invalid Results

Always follow the directions in this User Manual when you store, handle, and operate the Cue Health Monitoring System.

Some reasons for incorrect or invalid results are:

- Storing or operating the Cue Cartridge Reader in temperatures that are too low or too high. See “Technical Specifications” in Chapter 8 for more details.
- Storing or operating the Cue Cartridge Reader at altitudes that are too high. See “Technical Specifications” in Chapter 8 for more details.
- Dropping the Cue Health Monitoring System.
- Using a damaged Cue Health Monitoring System.

Initiate Test

 To Initiate a Test:

1. Launch the **Cue Health App** on your mobile smart device.



Cue Health

The “Login” screen is displayed by the Cue Health App after launch.

2. Log into your Cue Account.

The “Dashboard” screen is displayed by the Cue Health App after successful account login.

3. On the “Dashboard” screen, tap on “**+ BEGIN NEW TEST**”.

4. Follow on-screen instructions to run a test.

After the test is complete, the Cartridge Reader will automatically go into standby mode.

ⓘ *If two or more Cartridge Readers are paired, you must identify the Reader you want to use by its MAC address. See “Checking the MAC Address of a Connected Cue Cartridge Reader” in Chapter 5 for more details.*

Chapter 5

Cue Health Monitoring System Management

Charging the Cue Cartridge Reader

 To Charge your Cue Cartridge Reader:

1. Plug the Cue Power Adapter into wall power.
2. Connect Cue Charging Cable to the USB port of the Cue Power Adapter.
3. Connect the other end of the Cue Charging Cable to the USB port of the Cue Cartridge Reader to start charging.
4. You may also charge the Cue Cartridge Reader by placing it on top of the Cue Wireless Charging Base. Make sure the Cue Wireless Charging Base is connected to power.

When you connect or disconnect the Cue Charging Cable, the lights on the Reader will light up one-by-one (sequentially) and then flash to tell you the charge level.



Lights illuminate sequentially




Battery is 80% charged




Battery is 20% charged

*Green indicates flashing light


Account Settings

 To Access Your Account Settings:

1. When logged into your Cue Account, access the “Dashboard” screen by tapping on the home button  at the bottom of the screen.
2. Tap on “**My Account**”.
3. Tap on “**Settings**”.
4. Within the “**Settings**” menu, you can:
 - Allow Notifications
 - Allow Location Services
 - Enable Camera Access
 - Auto - Reconnect
 - Change Password
 - Delete Account

Pairing Additional Cue Cartridge Readers to Your Mobile Smart Device


 To Pair Additional Cue Cartridge Readers to your mobile smart device:


1. When logged into your Cue Account, access the “Dashboard” screen by tapping on the home button  at the bottom of the screen.
2. Tap on “**Manage Readers**”.
3. Confirm your mobile smart device Bluetooth is enabled.
4. Tap on “+”.
5. Follow on-screen instructions to pair the additional Cue Cartridge Reader.

Cue Cartridge Reader is now paired to the mobile smart device.

Connecting the Cue Cartridge Reader to the Cue Health App


 To Connect a Paired Cue Cartridge Reader to the Cue Health App:



 A Cue Cartridge Reader that is “Paired” to your mobile smart device can disconnect if the Cartridge Reader is out of Bluetooth range of the mobile smart device.

1. When logged into your Cue Account, access the “Dashboard” screen by tapping on the home button  at the bottom of the screen.
2. Tap on “**Manage Readers**”.
3. From the list of “**DISCONNECTED**” Cue Cartridge Readers, tap on the one you would like to connect to.

The indicator lights will flash when the Cue Cartridge Reader is connected to the Cue Health App.

Checking the MAC Address of a Connected Cue Cartridge Reader

 To Check the MAC address of the Connected Reader on the Cue Health App:



1. When logged into your Cue Account, access the “Dashboard” screen by tapping on the home button  at the bottom of the screen.
2. Tap on “**Manage Readers**”.
3. From the list of “**CONNECTED**” Cue Cartridge Readers, tap on the  next to the one you would like to check.

The MAC address will be displayed on the “Reader Information” screen.

4. Compare the MAC address printed on the bottom of the Cartridge Reader to the MAC address displayed on the “Reader Information” screen.

Disconnecting the Cue Cartridge Reader from the Cue Health App



 To Disconnect the Cue Health App from connected Cue Cartridge Readers:

1. When logged into your Cue Account, access the “Dashboard” screen by tapping on the home button  at the bottom of the screen.
2. Tap on “**Manage Readers**”.
3. From the list of “**CONNECTED**” Cue Cartridge Readers, tap on the  next to the one you would like to disconnect.
4. Look at the MAC address on the bottom of the Cartridge Reader. Confirm the MAC address on the screen matches the MAC address on the bottom of the Reader you want to disconnect.
5. Tap on “**DISCONNECT**”.

Cue Cartridge Reader is now disconnected from the Cue Health App.

Unpairing the Cue Cartridge Reader from Your Mobile Smart Device


 To Unpair the Cue Cartridge Reader from your mobile smart device:

1. When logged into your Cue Account, access the “Dashboard” screen by tapping on the home button  at the bottom of the screen.
2. Tap on “**Manage Readers**”.
3. From the list of “**CONNECTED**” and “**DISCONNECTED**” Cue Cartridge Readers, tap on the  next to the Reader you would like to unpair.
4. Tap on “**FORGET THIS READER**”.


Cue Cartridge Reader is now unpaired from the mobile smart device.

Managing User Account and Profiles

 To Manage User Account:


1. When logged into your Cue Account, access the “Dashboard” screen by tapping on the home button  at the bottom of the screen.
2. Tap on “**My Account**” for more options.

To Manage Profiles:

1. When logged into your Cue Account, access the Cue Dashboard by tapping on the home button  at the bottom of the screen.
2. Tap on "**Manage Profiles**".
3. Tap on the profile of interest and tap on "**VIEW**" for more options.

The "TEST HISTORY" and "MEDICATION HISTORY" of the profile can be viewed on the screen.


Forgot Your Password?

 To Retrieve your Password:

1. Launch the **Cue Health App** on your mobile smart device.
2. Tap on “**Forgot Password?**”
3. Follow the on-screen instructions.

Printing Your Test Results

 To Print your Test Results:


1. When logged into your Cue Account, access the “Dashboard” screen by tapping on the home button  at the bottom of the screen.


2. Tap on “**Manage Profiles**”.


3. Tap on the profile of interest and tap on “**VIEW**”.

The “TEST HISTORY” and “MEDICATION HISTORY” of the profile can be accessed on the screen.

4. From the “**TEST HISTORY**” list, tap on the test result of interest.


5. Tap on Print button at the top right corner of the screen. Then tap on “**PRINT**” at the bottom of the results display screen and choose the printer icon . Then tap Print at the top right of the screen.

 Printing Test Results from the Cue Health App requires that a printer be connected to the mobile smart device.

 If you print results in public places, you could be sharing your personal information.

Accessing Product Documentation

 To Access Product Documentation:

1. When logged into your Cue Account, access the “Dashboard” screen by tapping on the home button  at the bottom of the screen.
2. Tap on “**Help Center**” for options.

Chapter 6


Cleaning and Disinfecting


This section provides cleaning and disinfecting information for your Cue Health Monitoring System.


Cleaning and Disinfecting


The Cue Health Monitoring System should be cleaned and disinfected after each use. Wipe down with Clorox® Germicidal Wipes containing 0.55% sodium hypochlorite as the active ingredient.

 Do not spray any cleaning solution directly onto the Cue Cartridge Reader or into the Cartridge Port.

 Do not put any part of the Cue Health Monitoring System under water or any other liquid.

 Do not attempt to clean any internal parts.

 If part of your device becomes wet, wipe off all moisture and allow sufficient time for drying before use.

 Only Clorox Germicidal Wipes should be used. Other products have not been tested and should not be used. Follow manufacturer's instruction for handling and storage of wipes.

Chapter 7

Troubleshooting

In this chapter, you will learn about symbols and error messages displayed by the Cue Health App.

Pay attention to all symbols, messages, and indicator lights when you use the system. They give you important information to help you use the system correctly and safely.

If you have questions, contact Cue Health Customer Support at support@cuehealth.com or call toll-free at (833) CUE-TEST · (833) 283-8378.

Error Messages and Recommended Actions

Certain messages displayed by the Cue Health App indicate an error. An error message requires your attention and action.


The following table lists the Error Message and the Recommended Action.

Error Message	Recommended Action
App displays “Tilt Warning”	Position the Cue Cartridge Reader on top of a stable, flat, and level surface.
App displays “The battery on your cartridge reader is too low to run a test”	Connect the Cue Cartridge Reader to power. Use the Cue Health Monitoring System components/ accessories.

Error Message	Recommended Action
App displays “Testing Error” or “Cartridge Error”	Follow on-screen instructions.
App displays “Test Has Been Canceled”	Remove and dispose of the Cartridge. Take a new sample using a new test-specific Cue Sample Wand and use a new test-specific Cue Cartridge to repeat the test. See the Cue Health App on-screen instructions for additional details.

When to Use the Manual Reset Button

If the Cartridge Reader is not responding as described in this User Manual you must reset the Reader. Press and hold the Manual Reset Button for one second. Do not hold the Manual Reset Button for more than 3 seconds.

 Pressing the Manual Reset Button for 10 seconds will bring the Reader back to the out-of-the box settings. Wake the Reader by connecting it to power.

Chapter 8

Technical Information and Specifications

This section provides technical information on your Cue Health Monitoring System.

How the Cue Health Monitoring System Works

The Cue Health Monitoring System detects test-specific targets using electrochemical biosensor technology.

Technical Specifications

Cue Cartridge Reader Specifications

Power Supply	Input: 100-240V~, 50/60Hz, 0.2A Output: 5VDC, 1.5A, 7.5W
Dimensions	(3.0 in x 3.0 in x 1.5 in) (74 mm x 74 mm x 37 mm)
Weight	5.3 oz (150 g)
Display	Cue Health App on an iPhone 8+ (or later) mobile smart device screen
Operational Temperature	59°F (15°C) to 95°F (35°C)
Operational Humidity	10% to 100%
Operational Altitude	0 ft (0 m) to 8530 ft (2600 m)
Storage Temperature	39°F (4°C) to 100°F (38°C)

Storage Humidity	10% to 100%
Storage Altitude	< 8530 ft (2600 m)

 For test-specific Cue Cartridge technical specifications, refer to the test-specific Instructions for Use.

Compliance with International Standards

The Cue Health Monitoring System will be tested to the following standards:

- UL 61010-1. 3rd Edition.
- UL 61010-2-101. 2nd Edition.
- FCC Part 15B
- ICES-003
- IEC/EN 61326 Class B
- FCC Part 15.247
- UL 60950-1
- UL 62368-1

Disposing of Your Cue Health Monitoring System and Components

Dispose of used products according to regulations applicable in your country. For information about the correct method of disposal, contact your local authorities.

Chapter 9

Warranty and Supplies

Manufacturer's One Year Warranty

Cue Health Inc. warrants your new Cue Health Monitoring System will be free from defects in materials and workmanship for a period of one (1) year from the date of the original purchase. If during this time the Cue Health Monitoring System does not work properly because of a defect in materials or workmanship, Cue Health Inc. agrees to replace free of charge any and all parts proven to be defective and subject to warranty. This warranty only applies to the original purchaser of the Cue Health Monitoring System.

Supplies and Accessories

Cue Health Monitoring System supplies and accessories are available by calling toll-free at (833) CUE-TEST • (833) 283-8378.

